



Figure 1A. Supplementary. Karyotype Analysis

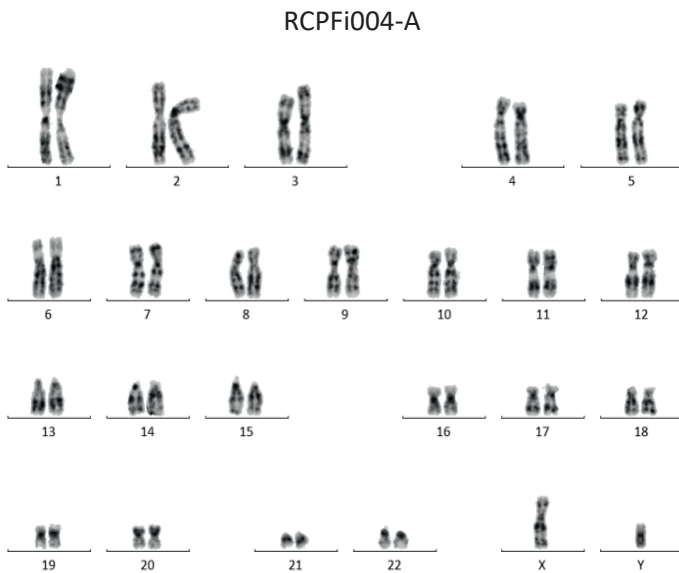

RCPFi005-A

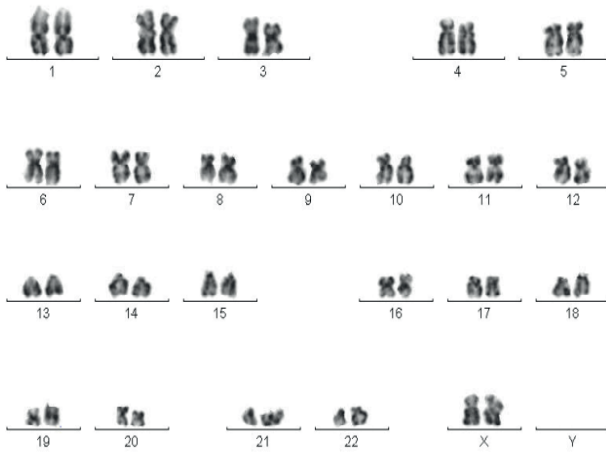

RCPFi006-A

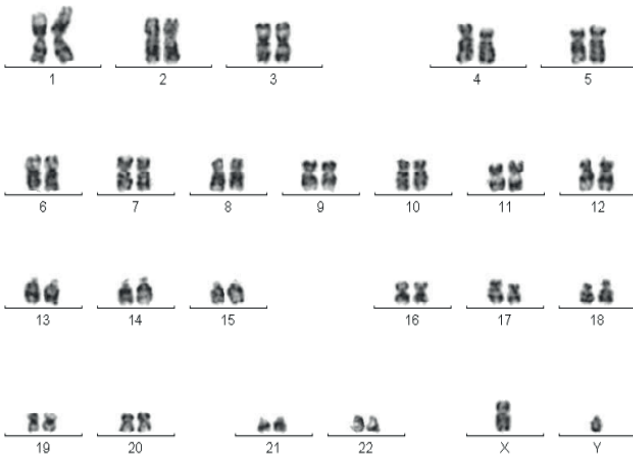


Figure 1B. Supplementary. Mycoplasma Result

Mycoplasma test by MycoAlert™ PLUS 27/11/2020	
Sample	Read B/Read A
Positive Control	2.33
Neagative Control	0.3
RCPFi004-A	0.37
RCPFi005-A	0.64
RCPFi006-A	0.5